

explore

LUNA[®]
OMEGA

Luna Omega C18

Application eBook

Your Go-To C18:

- Greater separation muscle
- Better peak shape through an inert foundation
- Extreme ruggedness and dependability



www.phenomenex.com/LunaOmega

phenomenex[®]

Luna Omega

Cutting Edge Fully Porous Silica Particle

Luna® is one of the most recognized HPLC brands on the market, delivering high efficiency, ruggedness, reproducibility, and dependability for a wide range of analyses. The new Luna Omega builds upon this legacy with an innovative yet rugged silica particle architecture, designed and manufactured by Phenomenex based on more than 20 years of applied knowledge, invention, and customer experience.




Novel Design and Manufacturing Process

Within the novel manufacturing process of Luna Omega silica, we implement a proprietary processing technique to gain greater particle inertness, a stronger particle morphology, and more consistent porosity.



Thermal Modified Pore Structure

Most importantly, through our proprietary process, we eliminate micropores, further improving column efficiency, inertness, and reproducibility.

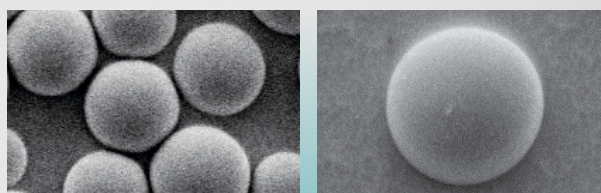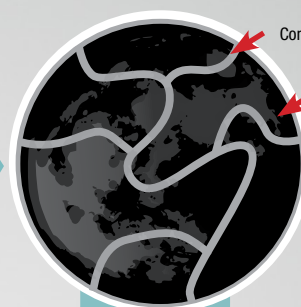

Enhanced with 20 Years of Technology, Innovation, and Experience

One of the world's leading HPLC brands, now enhanced for incredible LC performance! Luna Omega LC columns culminate 20 years of technological prowess, advancements, and innovation from Phenomenex!

With **astounding efficiency levels**, highly **versatile selectivities**, and **trusted accuracy**, Luna Omega columns will take your LC experience to a new level.



Luna® Omega UHPLC columns
will boost your LC instrumentation!

Table of Contents

Omega	Astounding Performance	p. 4
	Separation Muscle	p. 5
	Inert Foundation	p. 6
	Reproducible and Scalable	p. 7
C18	Selectivity Highlight Luna Omega C18	p. 8
	Small and Large Compound Mixtures	p. 9
	Small Molecule Organic Compounds	p. 10
	C18 Application Highlights	pp. 11 - 13
	Application Highlights Overview	p. 14
	Ordering Information	p. 15






Astounding Performance

The undeniably high efficiency levels found in each Luna Omega UHPLC/HPLC column provides you with the potential of huge gains in method performance. While traditional silica and hybrid fully porous particles claim high performance, when compared to Luna Omega, they drastically fall short and prevent UHPLC scientists from reaching their UHPLC potential.

UHPLC Efficiency Comparison

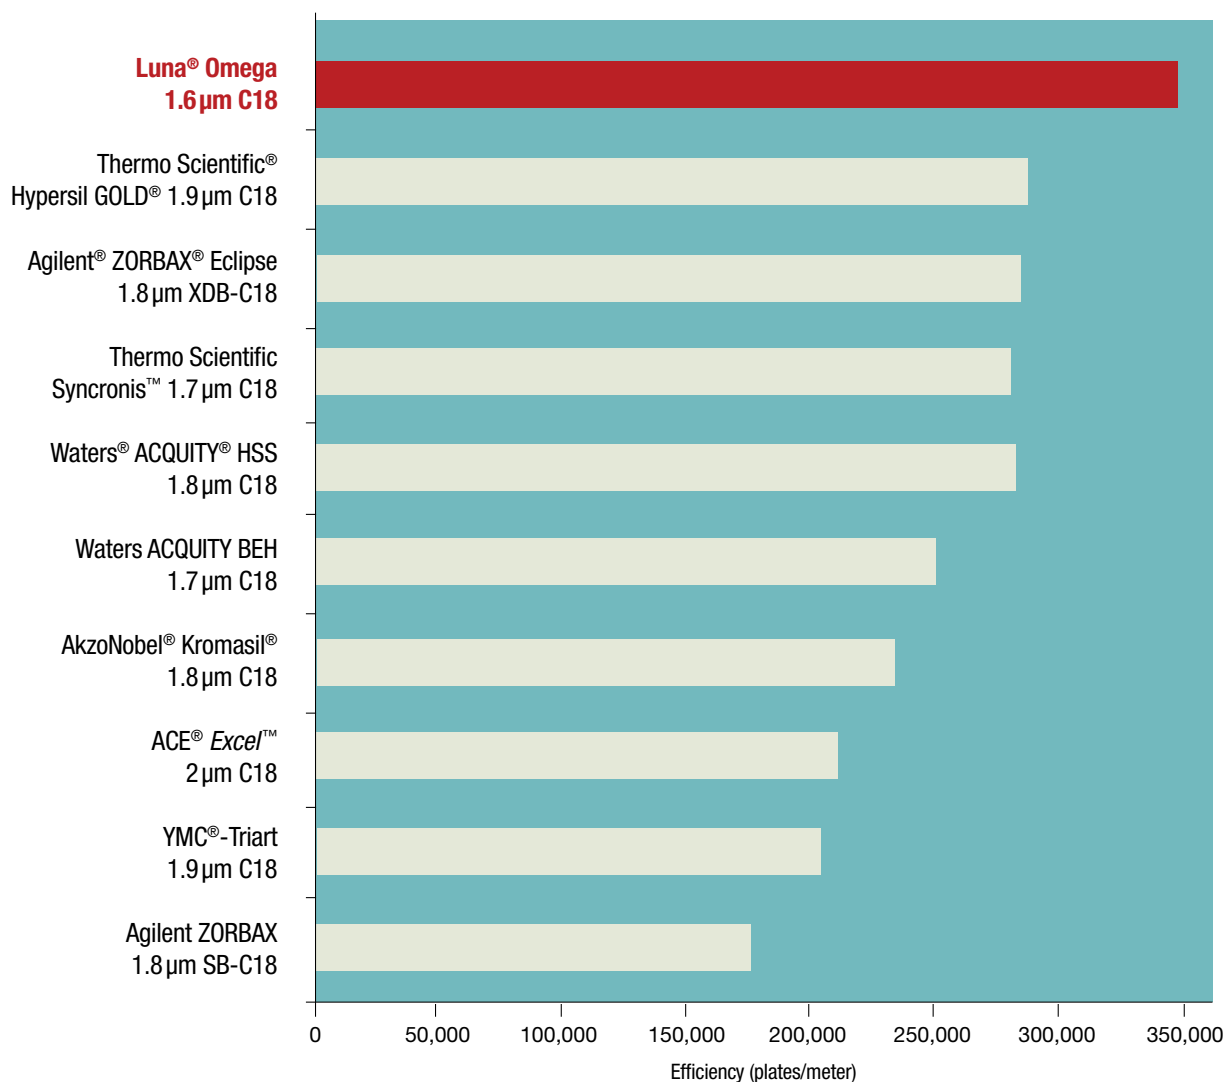


Conditions for all columns:
Dimension: 50 x 2.1 mm
Mobile Phase: Acetonitrile/Water (65:35)
Flow Rate: 0.5 mL/min
Temperature: Ambient
Detection: UV @ 254 nm
System: ACQUITY UPLC®
Sample: Naphthalene*


Comparative separations may not be representative of all applications.
*Efficiency (plates/meter) comparison is based on peak performance associated with the compound naphthalene for all columns.

Our industry leading bonding technologies in conjunction with high efficiency levels ensure excellent stationary phase coverage and improved separation power. Now, with Luna Omega 1.6, 3, or 5 μm , you can turn difficult separations into resolution that is reliable and repeatable.


Luna® Omega 1.6 μm C18

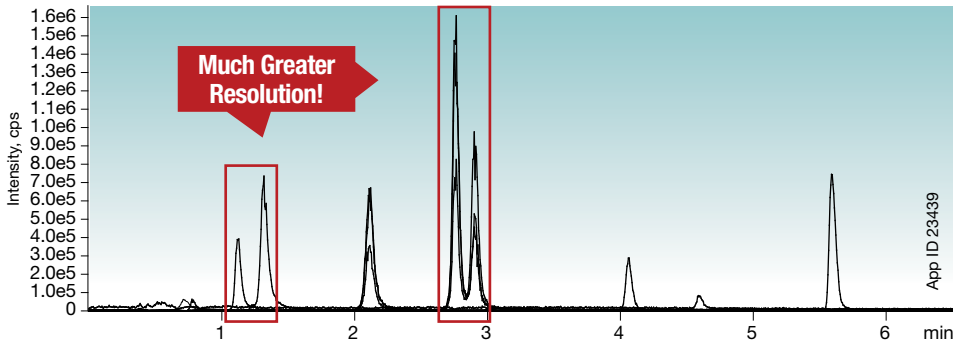

ACE® Excel™ 2 μm C18-AR

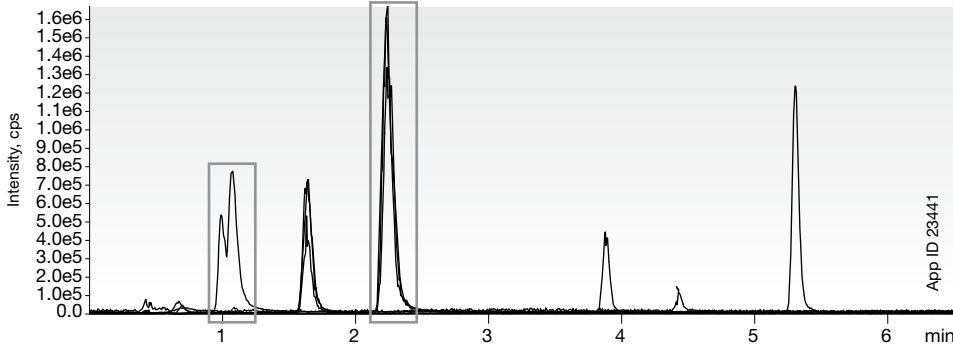

Agilent® ZORBAX® 1.8 μm XDB-C18

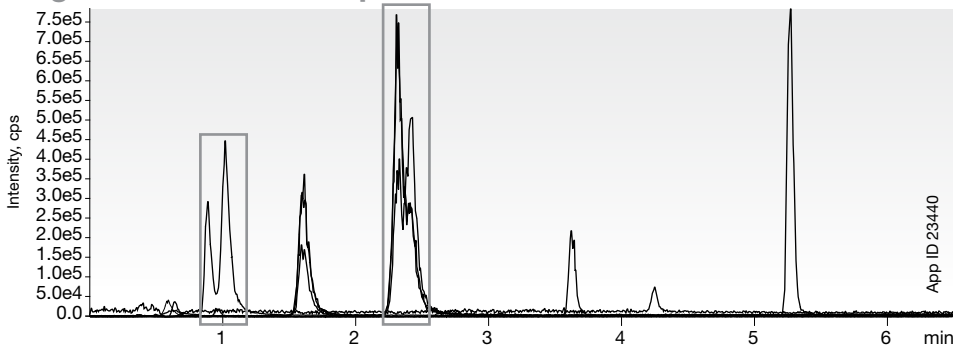

Conditions for all columns:

Columns: Luna Omega 1.6 μm C18
ZORBAX 1.8 μm XDB-C18
ACE Excel 2 μm C18-AR

Dimension: 50 x 2.1 mm

Mobile Phase: A: 0.1% Formic Acid in Water
B: 0.1% Formic Acid in Methanol

Gradient	Time (min)	% B
	0	3
	7	90

Flow Rate: 0.3 mL/min

Temperature: 30 °C


Detection: MS/MS

Sample: 1. Succinic acid
2. MMA
3. Glutaric acid
4. Methylsuccinate
5. Ethylmalonic acid
6. Hippuric acid
7. Homovanillic acid
8. Suberic acid


Comparative separations may not be representative of all applications.

Luna Omega HPLC and UHPLC columns contain a unique silica that is modified by using a proprietary, post-synthetic thermal treatment process to provide extraordinary mechanical strength and significantly greater inertness than traditional fully porous and hybrid materials. With this process, and our commitment to continuous improvement, the Luna Omega column is manufactured reproducibly from column-to-column, to batch-to-batch.


Luna® Omega 1.6µm C18

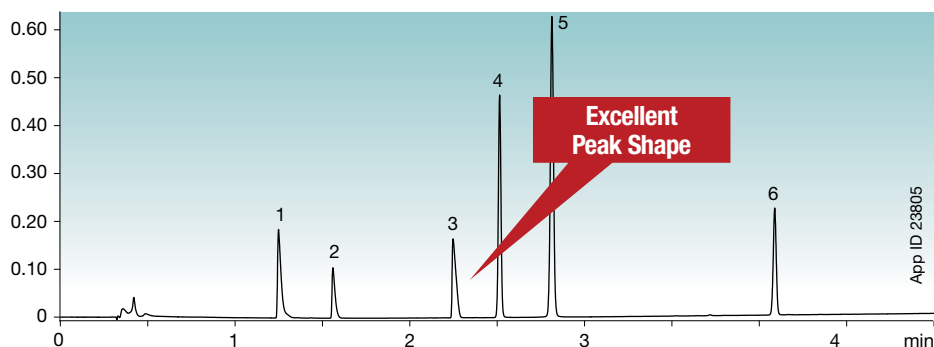

Waters® ACQUITY® BEH 1.7µm C18

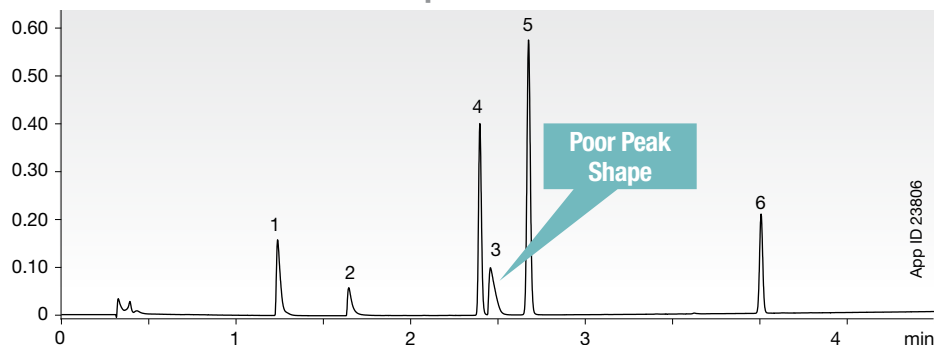

Thermo Scientific® Hypersil GOLD® 1.9µm C18

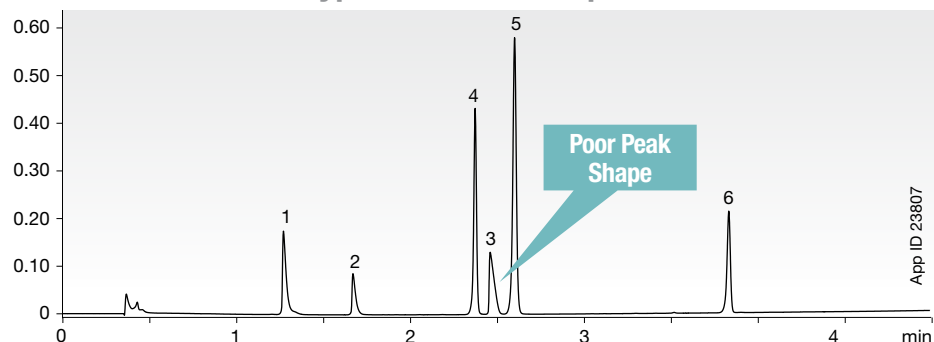

Conditions for all columns:

Columns: Luna Omega 1.6µm C18
ACQUITY BEH 1.7µm C18
Hypersil GOLD 1.9µm C18

Dimension: 50 x 2.1 mm

Mobile Phase: A: 0.1% Formic Acid in Water
B: 0.1% Formic Acid in Acetonitrile

Gradient:	Time (min)	% B
	0	5
	5	95
	6	95
	6.1	5
	8	5

Flow Rate: 0.4 mL/min
Temperature: Ambient
Detection: UV @ 254 nm

Sample: 1. Pindolol
2. Chlorpheniramine
3. Nortriptyline
4. 3-Methyl-4-nitrobenzoic acid
5. 5-Methyl salicylaldehyde
6. Hexanophenone

Comparative separations may not be representative of all applications.




By setting a new standard for reliability, the Luna® Omega C18 spans UHPLC and HPLC with a scalable range of high-performance particle sizes that will ensure that your developed methods are easily transferred. From single compound identification to complex impurity profiles, the Luna Omega C18 will serve as a pillar for your lab to count on day in and day out.

Batch-to-Batch Reproducibility Study


In this example, we compared three batches of Luna Omega C18 using all three different particle sizes on a complex QC Pharmaceutical representative sample.

Conditions for all columns:

- Mobile Phase:** A: Water with 0.1 % Formic Acid
B: Acetonitrile with 0.1 % Formic Acid
- Temperature:** 30 °C
- Detection:** UV @ 254 nm
- Injection Volume:** 5 µL
- Sample:** 5 mg/mL of Chlorhexidine and Related Substances



Luna Omega 5 µm C18
Impurity Profile 3 Batch Comparison

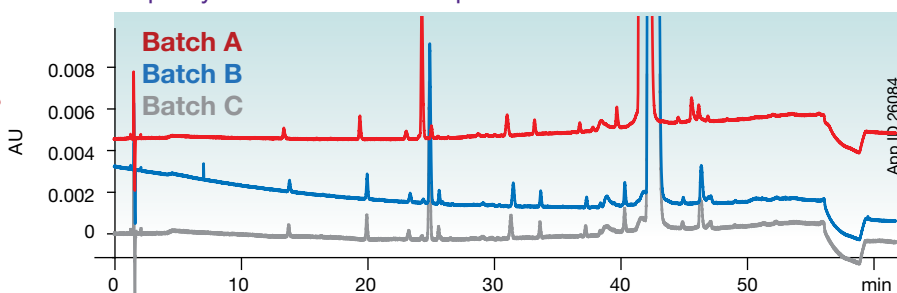


Column: Luna Omega 5 µm C18
Dimension: 250 x 4.6 mm
Part No.: 00G-4785-E0

Gradient:	Time (min)	% B
	0	2
	2.5	2
	52.5	35
	55	35
	57.5	2
	62.5	2

App ID 26084




Luna Omega 3 µm C18
Impurity Profile 3 Batch Comparison

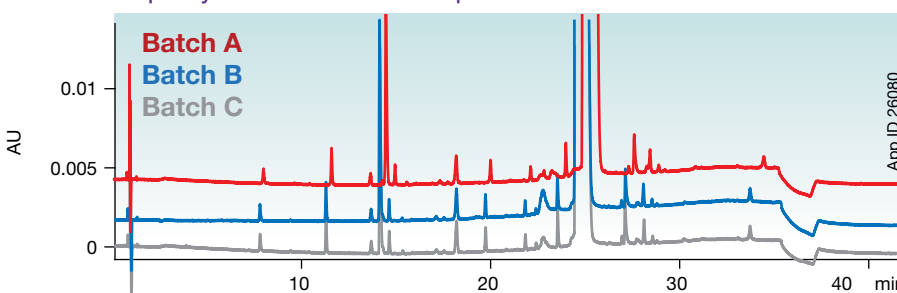


Column: Luna Omega 3 µm C18
Dimension: 150 x 4.6 mm
Part No.: 00F-4784-E0

Gradient:	Time (min)	% B
	0	2
	1.5	2
	31.5	35
	34.5	35
	36	2
	42	2

App ID 26080



Luna Omega 1.6 µm C18
Impurity Profile 3 Batch Comparison

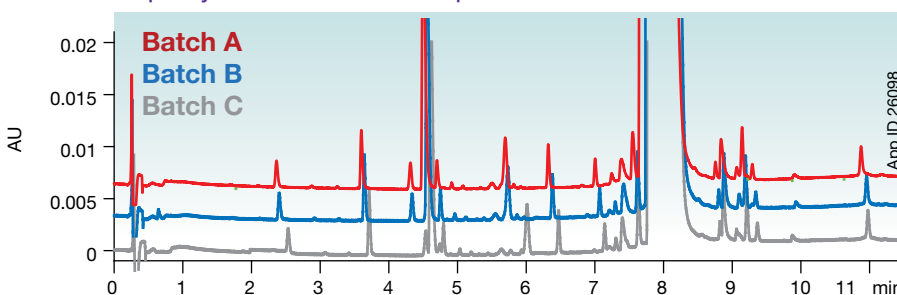

Column: Luna Omega 1.6 µm C18
Dimension: 50 x 2.1 mm
Part No.: 00B-4742-AN

Gradient:	Time (min)	% B
	0	2
	0.5	2
	10.5	35
	11.5	35
	12	2
	14	2

App ID 26098


Ω Selectivity Highlight Luna Omega C18

Selectivity Highlight Luna Omega C18

Luna® Omega C18 is an excellent first choice for chromatographers who are just starting method development or attempting to improve upon existing chromatographic results with other C18s. With its higher performance potential, excellent retention profile, and greater inertness, the Luna Omega C18 was designed to be the new reproducible, all-purpose HPLC/UHPLC solution for all industries.

Phase	C18
Particle Size	1.6, 3, 5 μm
Pore Size	100 Å
pH Range	1.5 - 8.5*
Surface Area	260 m ² /g
Carbon Load	11 %
Pressure Limit	1034/600 bar**
USP Listing	L1


*pH stability under gradient conditions. pH stability is 1.5-10 under isocratic conditions.
**1.6 μm Luna Omega columns are pressure stable up to 1,034 bar and 3 or 5 μm are stable up to 600 bar.

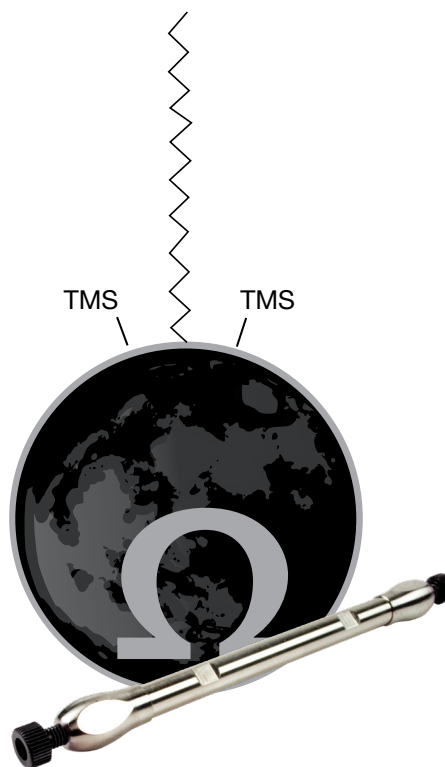

Greater Retention and Better Results

Higher efficiency levels in combination with excellent stationary phase coverage and greater particle inertness, translates to improved separation power for you. Now you can utilize the greater retention of Luna Omega C18 to tackle both easy and difficult separations.

Luna Omega 1.6 μm C18

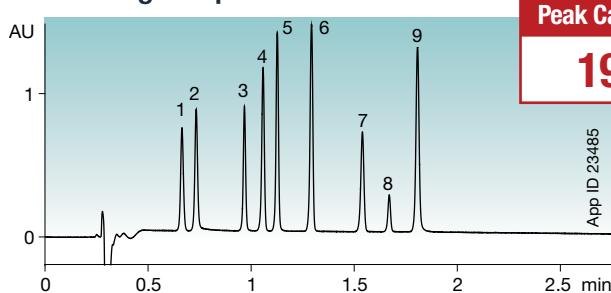


Peak Capacity

196

Greater Peak Capacity and Retention

Waters® ACQUITY® BEH 1.7 μm C18

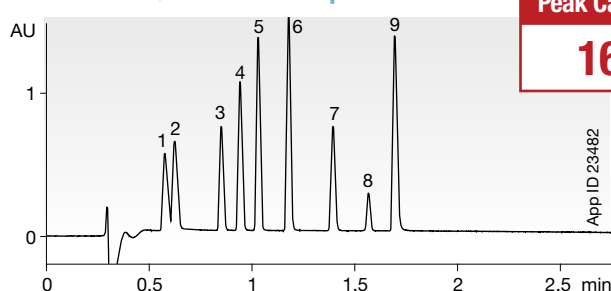

Peak Capacity

160

Conditions for all columns:

Columns: Luna Omega 1.6 μm C18
ACQUITY BEH 1.7 μm C18

Dimension: 50 x 2.1 mm

Mobile Phase: A: 0.1 % Formic Acid in Water
B: 0.1 % Formic Acid in Acetonitrile

Gradient:	Time (min)	% B
	0	10
	3	55
	3.5	55
	3.51	10
	5	10

Flow Rate: 0.4 mL/min

Temperature: Ambient

Detection: UV @ 205 nm


Sample: 1. Acetaminophen
2. 4-Aminobenzoic Acid
3. 4-Hydroxybenzoic Acid
4. 2-Acetaminophenol
5. 3-Hydroxybenzoic Acid
6. Salicylicamide
7. Phenol
8. Benzoic Acid
9. Salicylic Acid

Comparative separations may not be representative of all applications.

Small and Large Compound Mixtures

Strong and focused hydrophobic retention, incredible efficiency and valuable inertness of Luna® Omega C18 columns make them an excellent choice for small mixtures of compounds differing in hydrophobicity as well as large mixtures of compounds like impurity/degradation profiles and peptide maps.

Phenols

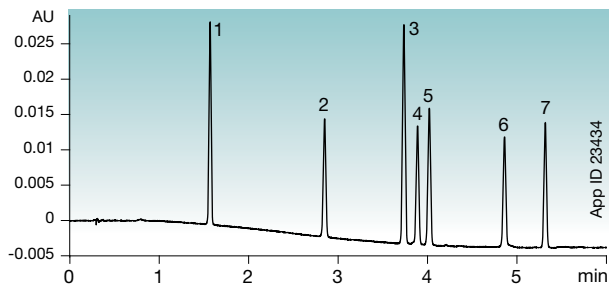


Columns: Luna Omega 1.6µm C18
Dimension: 50 x 2.1 mm
Part No.: 00B-4742-AN
Mobile Phase: A: 0.1% Formic Acid in Water
 B: 0.1% Formic Acid in Acetonitrile
Gradient:

Time (min)	% B
0	5
6	50
7	50
7.1	5
9	5

Flow Rate: 0.4 mL/min
Temperature: 22°C
Detection: UV @ 270 nm
Sample: 1. 3-Hydroxyphenol
 2. Phenol
 3. 4-Nitrophenol
 4. 4-Methylphenol
 5. 2-Methylphenol
 6. 2,4-Dimethylphenol
 7. 1-Naphthol

Synthetic Cannabinoids

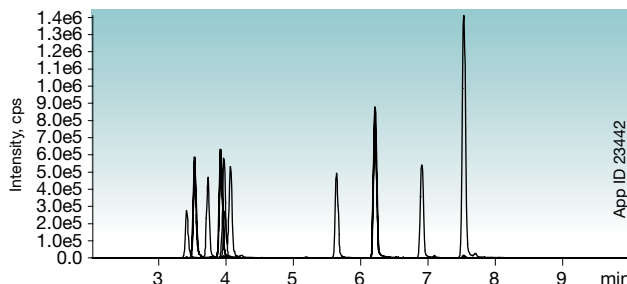


Columns: Luna Omega 1.6µm C18
Dimension: 50 x 2.1 mm
Part No.: 00B-4742-AN
Mobile Phase: A: 0.1% Formic Acid in Water
 B: 0.1% Formic Acid in Acetonitrile
Gradient:

Time (min)	% B
0	50
6	100

Flow Rate: 0.3 mL/min
Temperature: 30°C
Detection: MS/MS (SCIEX® API 4000™)
Sample: 1. JWH-073 Butanoic acid metabolite
 2. JWH-073 3-hydroxybutyl metabolite
 3. JWH-018 Pentanoic acid metabolite
 4. JWH-073 4-hydroxybutyl metabolite
 5. JWH-018 4-hydroxypentyl metabolite
 6. AM-2201 4-hydroxypentyl metabolite
 7. JWH-018 5-hydroxypentyl metabolite
 8. AM-694
 9. AM-2201
 10. JWH-073
 11. JWH-018

OTC Drug - Pill Formulation Profile

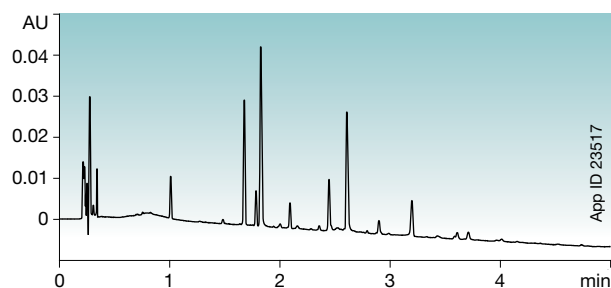


Columns: Luna Omega 1.6µm C18
Dimension: 50 x 2.1 mm
Part No.: 00B-4742-AN
Mobile Phase: A: 20 mM Potassium Phosphate pH 7.2
 B: Acetonitrile
Gradient:

Time (min)	% B
0	5
5	70
6	70
6.1	5
8	5

Flow Rate: 0.4 mL/min
Temperature: Ambient
Detection: UV @ 254 nm
Sample: OTC Drug Pill

Peptide Map – Digested BSA

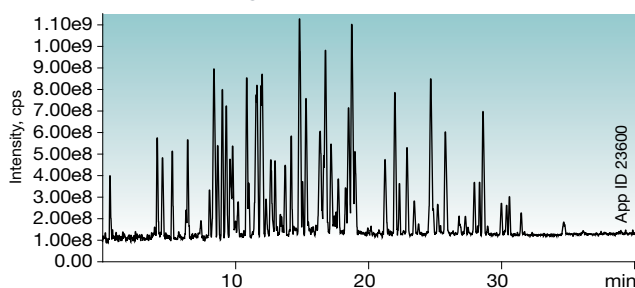


Columns: Luna Omega 1.6µm C18
Dimension: 100 x 2.1 mm
Part No.: 00D-4742-AN
Mobile Phase: A: 0.1% Formic Acid in Water
 B: 0.1% Formic Acid in Acetonitrile
Gradient:

Time (min)	% B
0	3
50	50
50.1	3

Flow Rate: 0.4 mL/min
Temperature: 40°C
Detection: MS/MS (SCIEX API 4000)
Sample: Tryptic digest of BSA

Comparative separations may not be representative of all applications.

Sildenafil Citrate RS and Sildenafil N-Oxide USP System Suitability Solution on Luna® Omega 5 µm C18

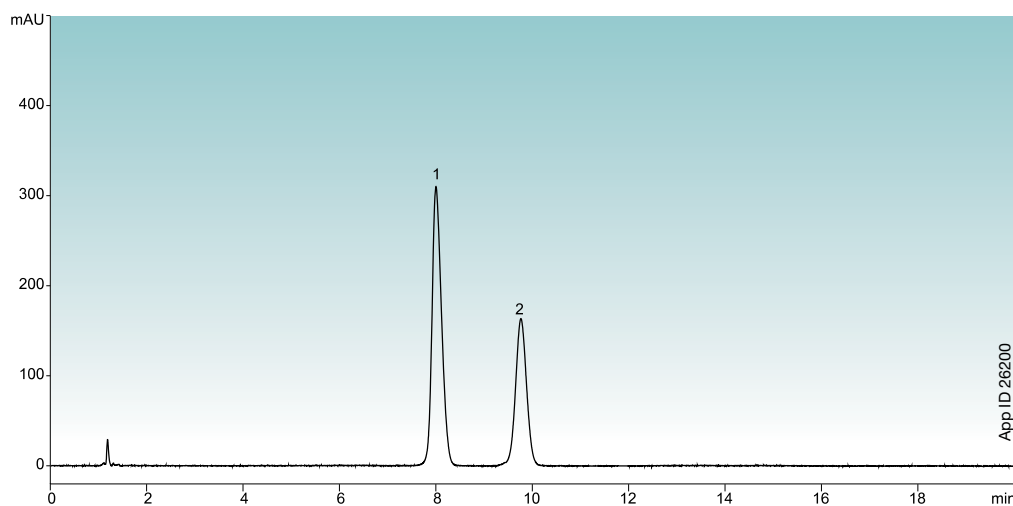


Columns: Luna Omega 5 µm C18
Dimension: 150 x 4.6 mm
Part No.: 00F-4785-E0
Elution Type: Isocratic
 Find the full elution online at www.phenomenex.com/Application/Detail/26200
Gradient:

Time (min)	% B
20	0

Flow Rate: 1.4 mL/min
Temperature: 30 °C
Detection: UV @ 290 nm
Sample: 1. Sildenafil citrate
 2. Sildenafil N-Oxide

Lisinopril Ph. Eur Reference Solution A+B+C+D on Luna Omega 5 µm C18

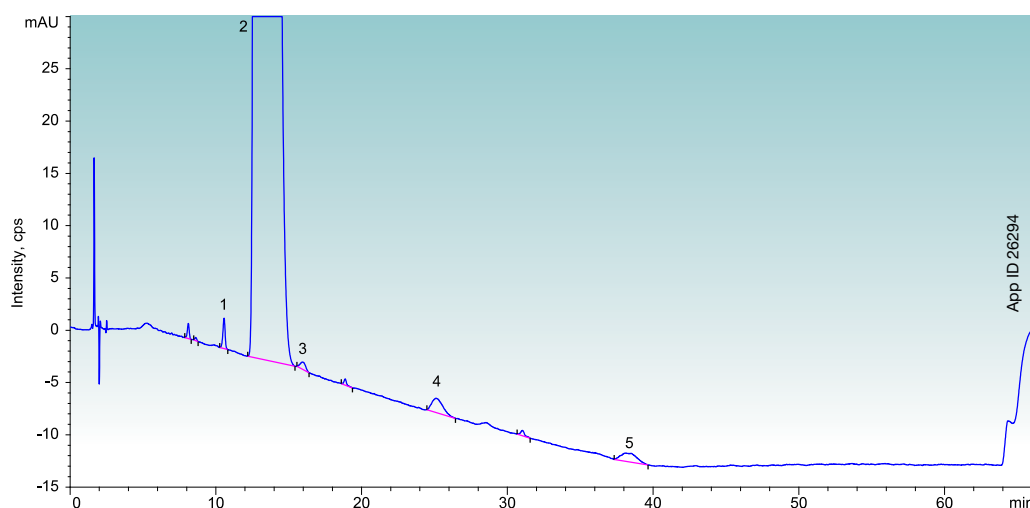

Columns: Luna Omega 5 µm C18
Dimension: 250 x 4.6 mm
Part No.: 00G-4785-E0
Elution Type: Gradient
 Find the full elution online at www.phenomenex.com/Application/Detail/26294
Gradient:

Time (min)	% B
0	0
2	0
37	100
62	100
62.5	0
66	0

Flow Rate: 1.4 mL/min
Temperature: 30 °C
Detection: UV @ 290 nm
Sample: 1. Impurity A
 2. Lisinopril
 3. Impurity E
 4. Impurity F
 5. Impurity G

Ph. Eur. Monograph 401: Levothyroxine Sodium

The suitability of this Luna Omega reversed phase HPLC column for the analysis of related substances according to Ph. Eur. monograph 401 and effect of adapting the flow rate according to the allowable adjustments of chapter 2.246 of the European Pharmacopoeia is shown here. System suitability requires a resolution of greater than 5 for the separation of impurity A and Levothyroxine.

Figure 2a: Reference **a on Luna® Omega 3 µm C18 with flow rate 1.0 mL/min**

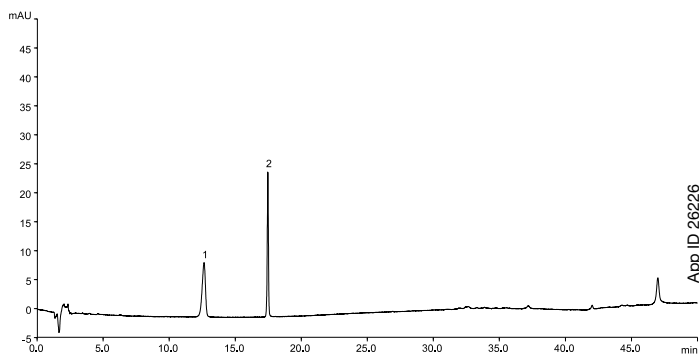


Figure 2b: Reference **d on Luna Omega 3 µm C18 with flow rate 1.0 mL/min**

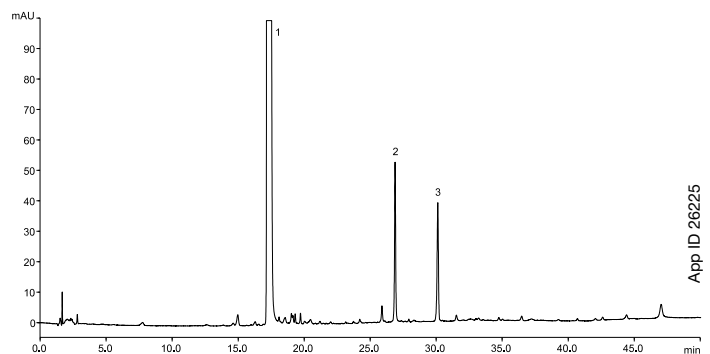


Figure 3a: Reference **a on Luna Omega 3 µm C18 with flow rate 1.32 mL/min**


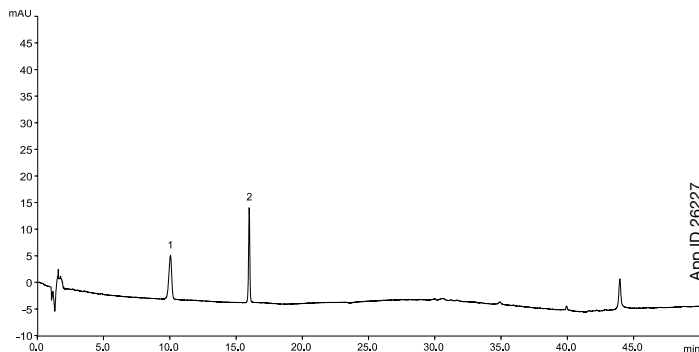


Figure 3b: Reference **d on Luna Omega 3 µm C18 with flow rate 1.32 mL/min**

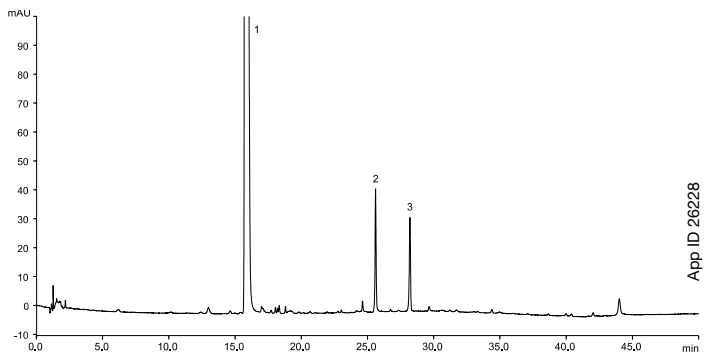

HPLC Conditions

Columns: Luna Omega 3 µm C18

Dimension: 150 x 4.6 mm

Part No.: 00F-4874-E0

Elution Type: A: 1.97 g phosphoric acid in 2 L water
B: 1.97 g phosphoric acid in 2 L acetonitrile

Gradient	Time (min)	% B
	0	30
	10	30
	40	80
	50	80

Flow Rate: as indicated on the chromatograms

Temperature: 25 °C

Injection: 25 µL

System: Shimadzu® Nexera® XR

Detector: UV @ 225 nm


See the full application note online at

www.phenomenex.com/TN77471120

Ω C18 Application Highlight

Rapid Analysis of 125 Pesticides from Groundwater by UHPLC-MS/MS

With this application, 125 pesticides and degradants can be quantified at approximately 10 ng/L in groundwater using UHPLC-MS/MS with a Luna® Omega 1.6 µm C18 column. The high resolution afforded by the Luna Omega C18 gives great separation, allowing the mass spectrometer to maximize dwell time and achieve very low detection limits in a short run of 8 minutes.

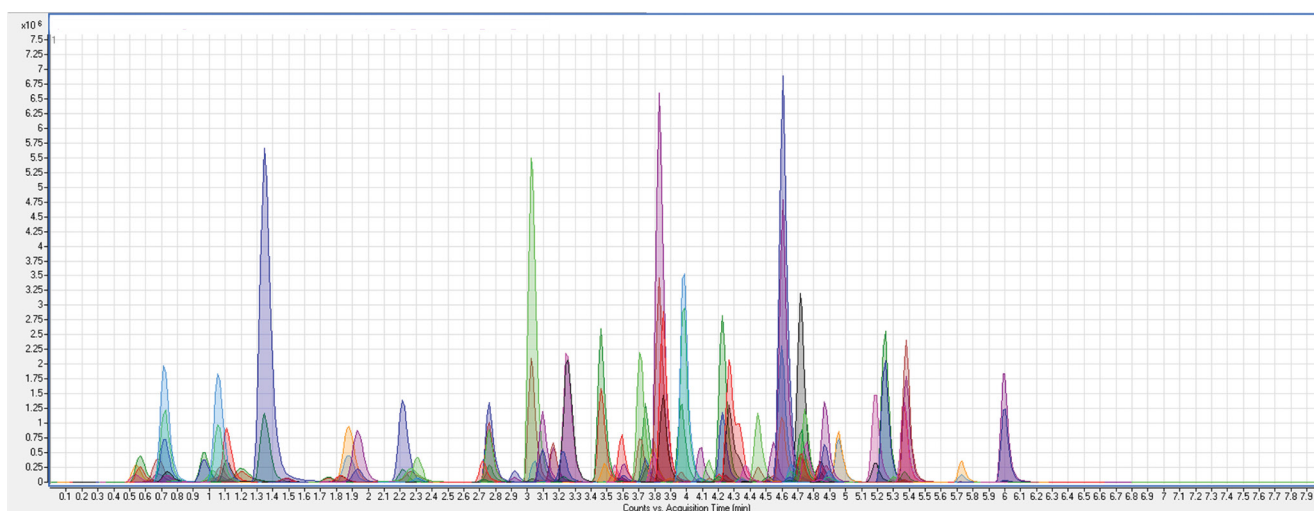

Column: Luna Omega 1.6 µm C18
Dimensions: 50 x 2.1 mm
Part No.: 00B-4742-AN
Mobile Phase: A: 2.5 mM Ammonium acetate + 0.05% Acetic acid in water
B: 0.05% Acetic acid in acetonitrile
Gradient:

Time (min)	% B
0	15
0.5	15
2.5	40
5.75	75
6.25	100
7	100
7.1	15
8	15

Injection: 75 µL- Direct Inject
Flow Rate: 0.55 mL/min
Temperature: 45 °C
Detection: Agilent® 6495 Triple Quadrupole LC-MS
Sample: 125 Pesticides and Degradants (see link below)

See the full application note online at


www.phenomenex.com/TN45280816



Analysis of Synthetic Cathinones (Bath Salts) from Urine and Whole Blood by LC-MS/MS

This application illustrates the separation of 5 common synthetic cathinones using a Luna® Omega 1.6 µm C18 UHPLC column. Luna Omega columns contain a unique silica which is modified using a proprietary, post-synthetic thermal treatment process to provide extraordinary mechanical strength and significantly greater inertness than traditional fully porous and hybrid materials. This greatly minimizes any secondary interactions that negatively affect peak shape, allowing for greater method accuracy.

Extracted Ion Chromatogram of Bath Salts in Whole Blood

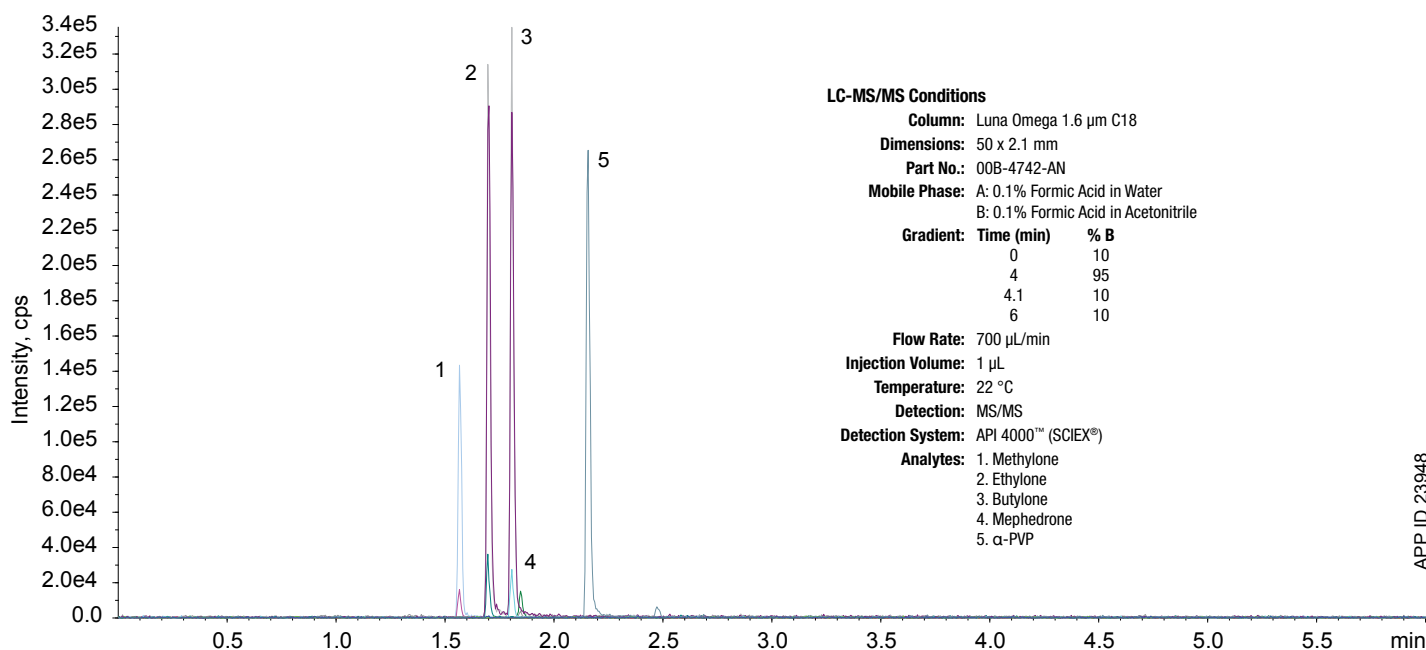

LC-MS/MS Conditions

Column: Luna Omega 1.6 µm C18
Dimensions: 50 x 2.1 mm
Part No.: 00B-4742-AN
Mobile Phase: A: 0.1% Formic Acid in Water
 B: 0.1% Formic Acid in Acetonitrile
Gradient:

Time (min)	% B
0	10
4	95
4.1	10
6	10

Flow Rate: 700 µL/min
Injection Volume: 1 µL
Temperature: 22 °C
Detection: MS/MS
Detection System: API 4000™ (SCIEX®)
Analytes: 1. Methylone
 2. Ethylone
 3. Butylone
 4. Mephedrone
 5. α-PVP

APP ID 23948

Sample Preparation

Solid Phase Extraction (SPE)

Cartridge:	Strata®-X-Drug B
Part No.:	8B-S128-UCH
Condition:	1 mL each of methanol, DI water, and 100 mM sodium acetate
Load:	Load pretreated sample
Weak Wash:	2 mL of 100 mM sodium acetate (pH 5.0)
Strong Wash:	1 mL of methanol
Dry Down:	2 minutes at >10" hg
Elute:	3 mL of ethyl acetate: IPA: ammonium hydroxide (70:20:10)
Evaporate:	to 500 µL and add 100 µL of HCl:methanol (20:80), evaporate to dryness under nitrogen
Reconstitute:	100 µL of methanol

Pretreatment

Urine	Add 2 mL of 100 mM sodium acetate buffer (pH 5.0) and 50 µL of internal standards (@10 ppm) to 2 mL of urine
Whole blood	1. Add 2 mL of ice cold methanol:acetonitrile (50:50) and 20 µL of internal standards (@10 ppm) and 2 mL of 100 mM sodium acetate to 1 mL of blood. 2. Centrifuge at 4700 rpm 10 °C for 5 min 3. Transfer supernatant for SPE

Q1	Q2	Analyte	Retention Time (min)
208.1	160.2	Methylone	1.56
222.3	174.1	Ethylone	1.69
222.3	174.1	Butylone	1.80
178.1	160.2	Mephedrone	1.84
232.4	91	α-PVP	2.15

See the full application note online at

www.phenomenex.com/TN48401216



Application Highlights Overview

Why chose Luna Omega columns?

- Greater separation muscle
- Better peak shape through an inert foundation
- Extreme ruggedness and dependability



Application Highlights

Environmental



Batch-to-Batch Comparison: Steroid Mixture on Luna Omega 3 µm C18



Scalability, Reproducibility, and Increased Separation Power of Luna Omega C18

Forensic/Toxicology



Scalability and Reproducibility of Luna Omega C18 for Acids, Bases and Neutrals



Inertness and Reproducibility of Luna Omega C18

Pharmaceuticals



Ph. Eur. Monograph 401: Levothyroxine Sodium on Luna C18(2) and Luna Omega C18



Rapid Analysis of 125 Pesticides from Groundwater by UHPLC-MS/MS using Luna Omega C18



Analysis of Synthetic Cathinones (Bath Salts) from Urine and Whole Blood by LC-MS/MS using Luna Omega C18



Luna Omega C18 Column-to-Column and Batch-to-Batch Reproducibility from HPLC to UHPLC



Demonstrating the Luna Omega C18's Reproducibility, Scalability – HPLC to UHPLC – 1.6 µm, 3 µm, and 5 µm



Comparison of Two High-Performance Particle Morphologies in the Separation of Hydrochlorothiazide and Chlorothiazide

Column Characteristics

Luna Omega Phases	Description	Particle Sizes (µm)	Pore Size (Å)	Surface Area (m ² /g)	Carbon Load (%)	pH Stability	Reversed Phase	HILIC
C18	C18 ligand optimized for improved peak shape	1.6, 3, 5	100	260	11	1.5 - 8.5*	☾	
Polar C18	Enhanced selectivity/retention for polar analytes without diminishing useful non-polar retention	1.6, 3, 5	100	260	9	1.5 - 8.5*	☾	
PS C18	Mixed-mode functionality offering enhanced retention of polar acids along with improved peak shape for strong bases	1.6, 3, 5	100	260	9	1.5 - 8.5*	☾	☾
Sugar	Combined amide/amino stationary phase and polar endcapping offers enhanced HILIC retention of sugars through multiple interaction mechanisms.	3	100	260	<2	2.0-7.0	☾	

* pH stability under gradient conditions. pH stability is 1.5 - 10 under isocratic conditions.

Ordering Information



1.6 µm Microbore Columns (mm)			
Phases	50 x 1.0	100 x 1.0	150 x 1.0
Polar C18	00B-4748-A0	00D-4748-A0	00F-4748-A0
PS C18	—	00D-4752-A0	—
C18	00B-4742-A0	00D-4742-A0	00F-4742-A0

1.6 µm Minibore Columns (mm)					SecurityGuard™ ULTRA Cartridges [†]
Phases	30 x 2.1	50 x 2.1	100 x 2.1	150 x 2.1	3/pk
Polar C18	00A-4748-AN	00B-4748-AN	00D-4748-AN	00F-4748-AN	AJO-9505
PS C18	00A-4752-AN	00B-4752-AN	00D-4752-AN	00F-4752-AN	AJO-9508
C18	00A-4742-AN	00B-4742-AN	00D-4742-AN	00F-4742-AN	AJO-9502

for 2.1 mm ID

3 µm Micro LC Columns (mm)							Trap Column
Phases	50 x 0.30	100 x 0.30	150 x 0.30	50 x 0.50	100 x 0.50	150 x 0.50	20 x 0.30
Polar C18	00B-4760-AC	00D-4760-AC	00F-4760-AC	00B-4760-AF	00D-4760-AF	00F-4760-AF	—
PS C18	00B-4758-AC	00D-4758-AC	00F-4758-AC	00B-4758-AF	00D-4758-AF	00F-4758-AF	05M-4758-AC

3 µm Minibore Columns (mm)					SecurityGuard Cartridges (mm)
Phases	30 x 2.1	50 x 2.1	100 x 2.1	150 x 2.1	4 x 2.0* /10 pk
Polar C18	00A-4760-AN	00B-4760-AN	00D-4760-AN	00F-4760-AN	AJO-7600
PS C18	00A-4758-AN	00B-4758-AN	00D-4758-AN	00F-4758-AN	AJO-7605
C18	—	00B-4784-AN	00D-4784-AN	00F-4784-AN	AJO-7611
SUGAR	—	00B-4775-AN	00D-4775-AN	00F-4775-AN	AJO-4496

for ID: 2.0-3.0 mm

3 µm MidBore™ Columns (mm)				SecurityGuard Cartridges (mm)
Phases	50 x 3.0	100 x 3.0	150 x 3.0	4 x 2.0* /10 pk
Polar C18	00B-4760-Y0	00D-4760-Y0	00F-4760-Y0	AJO-7600
PS C18	00B-4758-Y0	00D-4758-Y0	00F-4758-Y0	AJO-7605
C18	00B-4784-Y0	00D-4784-Y0	00F-4784-Y0	AJO-7611
SUGAR	—	—	00F-4775-Y0	AJO-4496

for ID: 2.0-3.0 mm

3 µm Analytical Columns (mm)					SecurityGuard Cartridges (mm)
Phases	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0* /10 pk
Polar C18	00B-4760-E0	00D-4760-E0	00F-4760-E0	00G-4760-E0	AJO-7601
PS C18	00B-4758-E0	00D-4758-E0	00F-4758-E0	00G-4758-E0	AJO-7606
C18	00B-4784-E0	00D-4784-E0	00F-4784-E0	00G-4784-E0	AJO-7612
SUGAR	—	00D-4775-E0	00F-4775-E0	00G-4775-E0	AJO-4495

for ID: 3.2-8.0 mm

5 µm Minibore and MidBore™ Columns (mm)							SecurityGuard Cartridges (mm)
Phases	50 x 2.1	100 x 2.1	150 x 2.1	50 x 3.0	100 x 3.0	150 x 3.0	4 x 2.0* /10 pk
Polar C18	00B-4754-AN	00D-4754-AN	00F-4754-AN	00B-4754-Y0	00D-4754-Y0	00F-4754-Y0	AJO-7600
PS C18	00B-4753-AN	00D-4753-AN	00F-4753-AN	00B-4753-Y0	00D-4753-Y0	00F-4753-Y0	AJO-7605

for ID: 2.0 - 3.0 mm

5 µm Analytical Columns (mm)					SecurityGuard Cartridges (mm)
Phases	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0* /10 pk
Polar C18	00B-4754-E0	00D-4754-E0	00F-4754-E0	00G-4754-E0	AJO-7601
PS C18	00B-4753-E0	00D-4753-E0	00F-4753-E0	00G-4753-E0	AJO-7606
C18	00B-4785-E0	00D-4785-E0	00F-4785-E0	00G-4785-E0	AJO-7612

for ID: 3.2-8.0 mm

5 µm Semi-Preparative Columns (mm)			SecurityGuard Cartridges (mm)
Phases	250 x 10	10 x 10** /3 pk	
Polar C18	00G-4754-N0		AJO-9519
PS C18	00G-4753-N0		AJO-9520

for ID: 9-16 mm

5 µm Axia™ Packed Preparative Columns (mm)					SecurityGuard Cartridges (mm)
Phases	50 x 21.2	100 x 21.2	150 x 21.2	250 x 21.2	15 x 21.2** /ea
Polar C18	00B-4754-PO-AX	00D-4754-PO-AX	00F-4754-PO-AX	00G-4754-PO-AX	AJO-7603
PS C18	00B-4753-PO-AX	00D-4753-PO-AX	00F-4753-PO-AX	00G-4753-PO-AX	AJO-7608
C18	—	—	—	00G-4785-PO-AX	—

for ID: 18-29 mm

5 µm Axia™ Packed Preparative Columns (mm) (cont'd)					SecurityGuard Cartridges (mm)
Phases	100 x 30	150 x 30	250 x 30	250 x 50	15 x 30.0* /ea
Polar C18	00D-4754-U0-AX	00F-4754-U0-AX	00G-4754-U0-AX	00G-4754-V0-AX	AJO-7604
PS C18	00D-4753-U0-AX	00F-4753-U0-AX	00G-4753-U0-AX	00G-4753-V0-AX	AJO-7609

for ID: 30-49 mm

[†] SecurityGuard ULTRA Cartridges require holder, Part No.: AJO-9000

^{**} SecurityGuard Analytical Cartridges require holder, Part No.: KJO-4282

^{***} SemiPREP SecurityGuard Cartridges require holder, Part No.: AJO-9281

^{††} PREP SecurityGuard Cartridges require holder, Part No.: AJO-8223

^{**††} PREP SecurityGuard Cartridges require holder, Part No.: AJO-8277

Luna Omega C18

Application eBook

explore

LUNA®
OMEGA



Australia

t: +61 (0)2-9428-6444
auinfo@phenomenex.com

Austria

t: +43 (0)1-319-1301
anfrage@phenomenex.com

Belgium

t: +32 (0)2 503 4015 (French)
t: +32 (0)2 511 8666 (Dutch)
beinfo@phenomenex.com

Canada

t: +1 (800) 543-3681
info@phenomenex.com

China

t: +86 400-606-8099
cninfo@phenomenex.com

Czech Republic

t: +420 272 017 077
cz-info@phenomenex.com

Denmark

t: +45 4824 8048
nordicinfo@phenomenex.com

Finland

t: +358 (0)9 4789 0063
nordicinfo@phenomenex.com

France

t: +33 (0)1 30 09 21 10
franceinfo@phenomenex.com

Germany

t: +49 (0)6021-58830-0
anfrage@phenomenex.com

Hong Kong

t: +852 6012 8162
hkinfo@phenomenex.com

India

t: +91 (0)40-3012 2400
indiainfo@phenomenex.com

Indonesia

t: +62 21 5010 9707
indoinfo@phenomenex.com

Ireland

t: +353 (0)1 247 5405
eirinfo@phenomenex.com

Italy

t: +39 051 6327511
italiainfo@phenomenex.com

Japan

t: +81 (0) 120-149-262
jinfo@phenomenex.com

Luxembourg

t: +31 (0)30-2418700
nlinfo@phenomenex.com

Mexico

t: 01-800-844-5226
tecnicomx@phenomenex.com

The Netherlands

t: +31 (0)30-2418700
nlinfo@phenomenex.com

New Zealand

t: +64 (0)9-4780951
nzinfo@phenomenex.com

Norway

t: +47 810 02 005
nordicinfo@phenomenex.com

Poland

t: +48 22 104 21 72
pl-info@phenomenex.com

Portugal

t: +351 221 450 488
ptinfo@phenomenex.com

Singapore

t: +65 800-852-3944
sginfo@phenomenex.com

Slovakia

t: +420 272 017 077
sk-info@phenomenex.com

Spain

t: +34 91-413-8613
esinfo@phenomenex.com

Sweden

t: +46 (0)8 611 6950
nordicinfo@phenomenex.com

Switzerland

t: +41 (0)61 692 20 20
swissinfo@phenomenex.com

Taiwan

t: +886 (0) 0801-49-1246
twinfo@phenomenex.com

Thailand

t: +66 (0) 2 566 0287
thaiinfo@phenomenex.com

United Kingdom


t: +44 (0)1625-501367
ukinfo@phenomenex.com

USA

t: +1 (310) 212-0555
info@phenomenex.com

☎ All other countries/regions

Corporate Office USA
t: +1 (310) 212-0555
info@phenomenex.com



www.phenomenex.com

Phenomenex products are available worldwide. For the distributor in your country/region, contact Phenomenex USA, International Department at international@phenomenex.com

Terms & Conditions

Subject to Phenomenex Standard Terms & Conditions, which may be viewed at www.phenomenex.com/TermsAndConditions.

Trademarks

Luna and Strata are registered trademarks and Axia, SecurityGuard, and MidBore are trademarks of Phenomenex. ACE is a registered trademark and Excel is a trademark of Advanced Chromatography Technologies Limited. Waters, ACQUITY, and UPLC are registered trademarks of Waters Technologies Corporation. Agilent and ZORBAX are registered trademarks of Agilent Technologies, Inc. Thermo Scientific is a registered trademark and Syncronis is a trademark of Thermo Fisher Scientific. Hypersil GOLD is a registered trademark of Thermo Hypersil-Keystone LLC. AkzoNobel and Kromasil are registered trademarks of AkzoNobel Pulp and Performance Chemicals AB. YMC is a registered trademark of YMC Co., Ltd. SCIEX is a registered trademark and API 4000 is a trademark of AB SCIEX Pte. Ltd. Shimadzu and Nexera are registered trademarks of Shimadzu Corporation.

Disclaimer

Phenomenex is not affiliated with Agilent Technologies, AkzoNobel, Thermo Fisher Scientific, YMC, or Waters Corporation.

Comparative separations may not be representative of all applicants.

Axia column and packing technology is patented by Phenomenex. U.S. Patent No. 7, 674, 383

Strata-X is patented by Phenomenex. U.S. Patent No. 7,119,145

SecurityGuard is patented by Phenomenex. U.S. Patent No. 6,162,362

CAUTION: this patent only applies to the analytical-sized guard cartridge holder, and does not apply to SemiPrep, PREP or ULTRA holders, or to any cartridges.

FOR RESEARCH USE ONLY. Not for use in clinical diagnostic procedures

© 2021 Phenomenex Inc. All rights reserved.